



RECOGNIZED COMPONENT Constructional Data Report (CDR)

1.0 Reference and Address					
Report Number	130501374SHA-001	Original Issued:	24-Jun-2013	Revised:	15-Aug-2013
Standard(s)	Medical electrical equipment, Part 1: General requirements for basic safety and essential performance (ANSI/AAMI ES60601-1 Issued: 2006/03/09: 2005 Version (R2012); with AMD C1: 2009, AMD C2: 2010 & CAN/CSA-C22.2 No.60601-1 Issued: 2008/02/01; with COR 2: 2011/06/01); Medical electrical equipment, Part 1-11: General requirements for basic safety and essential performance - Collateral Standard: Requirements for medical electrical equipment and medical electrical systems used in the home healthcare environment (ANSI/AAMI HA60601-1-11 Issue:2011/12/12 Ed:1).				
Applicant	GlobTek, Inc.		Manufacturer	GlobTek (Suzhou) Co., Ltd.	
Address	186 Veterans Dr. Northvale, NJ 07647 USA		Address	Building 4. No 76 JinLing East Road, Suzhou Industrial Park, Suzhou, JiangSu, 215021	
Country	USA		Country	China	
Contact	Hans Moritz		Contact	Demon Zhou	
Phone	(201)784-1000 Ext.253		Phone	86 512 6279 0301 Ext.189	
FAX	(201)784-0111		FAX	86 512 6279 0355	
Email	Moritzh@globtek.com		Email	demon.zhou@globtek.cn	

2.0 Product Description	
Product	Medical Power Supply
Brand name	GlobTek
Description	<p>Product covered by this report is medical power supply module, which can be used as a part of medical equipment. It is direct plug-in power adapter with interchangeable plug portion, which is Class II apparatus. It can be used with different plug types. The evaluation report of NEMA 1-15P plug type is also attached with this report. Two pieces of outer enclosure are enclosed with ultrasonic welding without screw.</p> <p>All the types are designed for continuous operation and no applied part is defined. Insulation between mains part and secondary circuits is evaluated as 2MOPP.</p>
Models	GT*41061-*** (The 1st "*" part can be 'M' or '-' or 'H'; The 2nd "*" part can be "01" to "18", with interval of 1; The 3rd "*" part can be "12", "18", "24" or "30"; The 4th "*" part can be "-0.1" to "-7.0" with interval of 0.1 or blank.)
Model Similarity	<p>GT*41061-***</p> <p>The 1st "*" part can be 'M' or '-' or 'H' for market identification and not related to safety. The 2nd "*" part denotes the rated output wattage designation, which can be "01" to "18", with interval of 1.</p> <p>The 3rd "*" part denotes the standard rated output voltage designation, which can be "12", "18", "24" or "30". These standard rated output voltage designations correspond to four isolated transformer models (See the appended table 8.10 for details). Each transformer model is identical in insulation construction including clearance and creepage except number of turns per coil.</p> <p>The 4th "*" part is optional, which can be "-0.1" to "-7.0" with interval of 0.1 to denote voltage deviation or blank to indicate no voltage different. The result by subtracting the deviation value from the standard rated output voltage denotes the rated output voltage, with a range of 5 - 30 volts.</p>
Ratings	<p>Input: 100-240V~, 50-60Hz, 0.6A; Output: Refer to illustration No.1 for details.</p>
Other Ratings	N/A

2.0 Product Description

Conditions of Acceptability	<p>The products covered in this Report are incomplete in construction features or limited in performance capabilities and are intended for use and evaluation in other products. Consideration should be given to the following when the component is used in or with another product.</p> <p>Scope of Power Supply evaluation defers the following clauses to be determined as part of the end product investigation:</p> <ul style="list-style-type: none">• 60601-1 Clause 7.5 (Safety Signs),• 60601-1 Clause 7.9 (Accompanying Documents are provided for some critical issue like technical data, safety warnings, necessary information to set up, but further evaluation is needed on end product level.),• 60601-1 Clause 8.11.5 (Mains Fuse with High Breaking Capacity),• 60601-1 Clause 9 (ME Hazard), except 9.1 and 9.3 are evaluated,• 60601-1 Clause 10 (Radiation),• 60601-1 Clause 11.7 (Biocompatibility),• 60601-1 Clause 14 (PEMS),• 60601-1 Clause 16 (ME Systems)• 60601-1 Clause 17 (EMC),• 60601-11 Clause 7.1 (Usability of the accompanying documents),• 60601-11 Clause 7.4 (Instructions for use),• 60601-11 Clause 11 (Protection against strangulation or asphyxiation),• 60601-11 Clause 12 (Additional requirements for EMC)• 60601-11 Clause 13 (Additional requirements for Alarm system),
-----------------------------	--

4.0 Critical Components						
Photo #	Item no. ¹	Name	Manufacturer/ trademark ²	Type / model ²	Technical data and securement means	Mark(s) of conformity ³
1, 12	1	Plastic enclosure & Blade holder material	ELECTRIC CO	SE1X	Min. V-1 at 1.5 mm thickness, 105°C	cURus
			LTD	C2950	Min. V-0 at 1.5 mm thickness, 75 °C	
			SABIC INNOVATIVE PLASTICS B V	CX7211 EXCY0098	Min. V-1 at 1.25 mm thickness, 85°C	
			TEIJIN CHEMICALS LTD	LN-1250P LN-1250G	Min. V-0 at 1.5 mm thickness, 115°C	
			CHI MEI Corporation	PA-765A	Min. V-1 at 1.5 mm thickness, 80 °C	
			CHI MEI Corporation	PC-540	Min. V-0 at 1.5 mm thickness, 70 °C	
3	2	Fuse (F1, F2) (F2 is optional)	Conquer Electronics Co., Ltd.	MST	T2A, 250V, Rated breaking capacity 100A	cURus
			Ever Island Electric Co., Ltd. and Walter Electric	2010	T2A, 250V, Rated breaking capacity 130A	
			Bel Fuse Ltd.	RST	T2A, 250V, Rated breaking capacity 100A	
			Cooper Bussmann LLC	SS-5	T2A, 250V, Rated breaking capacity 35A	
			Walter Electronic Co. Ltd.	ICP series	T2A, 250V, Rated breaking capacity 50A	
			Das & Sons International Ltd.	385T series	T2A, 250V, Rated breaking capacity 35A	
			Shenzhen Lanson Electronics Co. Ltd.	SMT	T2A, 250V, Rated breaking capacity 35A	
3	2a	Insulation tube used on the fuse (Only for fuse ICP model)	SHENZHEN WOER HEAT-SHRINKABLE MATERIAL CO LTD	RSFR RSFR-H RSFR-HPF	600V, 125°C	cURus
			QIFURUI ELECTRONICS CO	QFR-h	600V, 125°C	
			DONGGUAN SALIPT CO LTD	SALIPT S- 901-300 SALIPT S- 901-600	Min. 300V, 125°C	
			GUANGZHOU KAIHENG ENTERPRISE GROUP	K-2 (+) K-2 (CB)	Min. 300V, 125°C	
			CHANGYUAN ELECTRONICS (SHENZHEN) CO LTD	CB-HFT	Min. 300V, 125°C	

4.0 Critical Components						
Photo #	Item no. ¹	Name	Manufacturer/ trademark ²	Type / model ²	Technical data and securement means	Mark(s) of conformity ³
3	3	X capacitor (CX1) (Optional)	Cheng Tung Industrial Co., Ltd.	CTX	Max.0.47uF, 310Vac, 110°C, type X2	cURus
			Tenta Electric Industrial Co. Ltd.	MEX	Max.0.47uF, 250/275Vac, 100° C, type X2	
			Ultra Tech Xiphi Enterprise Co. Ltd.	HQX	Max.0.47uF, 275Vac, 110°C, type X2	
			Okaya Electric Industries	RE series	Max.0.47uF, 275Vac, 100°C, type X2	
			VISHAY Capacitors Belgium NV	F1772	Max.0.47uF, 310Vac, 110°C, type X2	
			Winday Electronic Industries Co., Ltd.	MPX	Max.0.47uF, 250/275/280/300/310Vac, 110° C, type X2	
			Dain Electronics Co., Ltd.	MPX, MEX and NPX	Max.0.47uF, 250/275/310Vac, 100°C, type X2	
			Sinhua Electronics (Huzhou) Co., Ltd.	MPX	Max.0.47uF, 310Vac, 110°C, type X2	
			Shunde Da Hua Electric Co., Ltd.	HD-MKP	Max.0.47uF, 250Vac, 105°C, type X2	
			Foshan Shunde Chuang Ge	MKP-X2	Max.0.47uF, 275Vac, 105°C, type X2	
			Hongzhi Enterprises Ltd.	MPX	Max.0.47uF, 275Vac, 100°C, type X2	
3	4	Varistor (MOV1) (optional)	JOYIN CO LTD	07N471K 10N471K 14N471K	Maximum continuous voltage: 300Vac	cURus, VDE
			CENTRA SCIENCE CORP	07D471K 10D471K 14D471K		
			THINKING ELECTRONIC INDUSTRIAL CO LTD	TVR07471K TVR10471K TVR14471K		
			SUCCESS ELECTRONICS CO LTD	SVR07D471K SVR10D471K SVR14D471K		
			CERAMATE TECHNICAL CO LTD	GNR07D471K GNR10D471K GND14D471K		
			BRIGHTKING (SHENZHEN) CO LTD	07D471K 10D471K 14D471K		
			LIEN SHUN ELECTRONICS CO LTD	07D471K 10D471K 14D471K		
			HONGZHI ENTERPRISES LTD	HEL-07D471K HEL-10D471K HEL-14D471K		
			GUANGXI NEW FUTURE INFORMATION INDUSTRY CO LTD	07D471K 10D471K 14D471K		

4.0 Critical Components						
Photo #	Item no. ¹	Name	Manufacturer/ trademark ²	Type / model ²	Technical data and securement means	Mark(s) of conformity ³
3	5	Y-Capacitor (CY1, CY2) (optional)	TDK-EPC CORPORATION	CD	Type Y1, max. 1000pF, min. 250V, min. 85°C	cURus
			SUCCESS ELECTRONICS CO LTD	SE SB	Type Y1, max. 1000pF, min. 250V, min. 125°C	
			MURATA MFG CO LTD	KX	Type Y1, max. 1000pF, min. 250V, min. 125°C	
			WALSIN TECHNOLOGY CORP	AH	Type Y1, max. 1000pF, min. 250V, min. 125°C	
			JYA-NAY CO LTD	JN	Type Y1, max. 1000pF, min. 250V, min. 125°C	
			HAOHUA ELECTRONIC CO	CT7	Type Y1, max. 1000pF, min. 250V, min. 125°C	
			HONGZHI ENTERPRISES LTD	Y	Type Y1, max. 1000pF, min. 250V, min. 85°C	
			JERRO ELECTRONICS CORP	JX-series	Type Y1, max. 1000pF, min. 250V, min. 85°C	
3	6	Optocoupler (U2) (Not shown)	LITE-ON Technology Corporation	LTV-817C	Ext. Cr: min. 8.0 mm; DTI: min. 0.6 mm; Thermal cycling test. Max. operating temp.: 115°C.	CB
			Everlight Electronics Co., Ltd.	EL817	Ext. Cr: min. 7.7 mm; DTI: min. 0.5 mm; Thermal cycling test. Max. operating temp.: 110°C.	
3	7	Line filter (LF1) (Optional)	GlobTek / BOAM / ZhongTong / HEJIA	NF00030	Class A	NR
3, 7- 12	8	Transformer (T1)	GlobTek / BOAM / ZhongTong	TF001 TF002 TF003 TF004	Class E, with critical component listed below	NR
3, 7- 12	8a	Bobbin	CHANG CHUN PLASTICS CO LTD	T375J T375HF	V-0, 150°C, thickness 0.45 mm min.	cURus
			SUMITOMO BAKELITE CO LTD	PM-9820		
			HITACHI CHEMICAL CO LTD	CP-J-8800		
3, 7- 12	8b	Insulating tape	3M COMPANY ELECTRICAL MARKETS DIV (EMD)	1350F-1 1350T-1	Min. 130°C	cURus
			BONDTEC PACIFIC CO LTD	370S		
			JINGJIANG YAHUA PRESSURE SENSITIVE GLUE CO LTD	PZ CT		
			JINGJIANG JINGYI ADHESIVE PRODUCT CO LTD	JY25-A		
			CHANG SHU LIANG YI TAPE INDUSTRY CO LTD	LY-XX		

4.0 Critical Components						
Photo #	Item no. ¹	Name	Manufacturer/ trademark ²	Type / model ²	Technical data and securement means	Mark(s) of conformity ³
3, 7-12	8c	Magnet wire (Primary winding)	PACIFIC ELECTRIC WIRE & CABLE (SHENZHEN) CO LTD	UEWN/U	130°C	cURus
			JUNG SHING WIRE CO LTD	UEW-4 UEY-2		
			JIANGSU HONGLIU MAGNET WIRE TECHNOLOGY CO LTD	2UEW/130		
			CHANGZHOU DAYANG WIRE & CABLE CO LTD	2UEW/130		
			WUXI JUFENG COMPOUND LINE CO LTD	2UEWB		
			JIANGSU DARTONG M & E CO LTD	UEW		
			SHANDONG SAINT ELECTRIC CO LTD	UEW/130		
			ZHEJIANG LANGLI ELECTRIC EQUIPMENTS CO LTD	UEW		
3, 7-12	8d	Triple-insulated wire (Secondary winding)	GREAT LEOFLON INDUSTRIAL CO LTD	TRW(B)	Min. 130°C	cURus
			COSMOLINK CO LTD	TIW-M		
			FURUKAWA ELECTRIC CO LTD	TEX-E		
			TOTOKU ELECTRIC CO LTD	TIW-2		
3, 7-12	8e	Pin-out support (PCB material) (Optional)	DONGGUAN DAYSUN ELECTRONIC CO LTD	DS2	Min. V-0, min 1.0 mm thickness, 130°C	cURus
			Various	Various	Min. V-1, min 1.0 mm thickness, min. 130°C	

4.0 Critical Components						
Photo #	Item no. ¹	Name	Manufacturer/ trademark ²	Type / model ²	Technical data and securement means	Mark(s) of conformity ³
3	9	PCB material	TECHNI TECHNOLOGY LTD	T2A T2B T4	Min 1.6 mm thickness, min. V-0, 130°C	cURus
			DONGGUAN HE TONG ELECTRONICS CO LTD	CEM1		
			CHEERFUL ELECTRONIC	03 03A		
			DONGGUAN DAYSUN ELECTRONIC CO LTD	DS2		
			SUZHOU CITY YILIHUA ELECTRONICS CO LTD	YLH-1		
			SHANGHAI AREX PRECISION ELECTRONIC CO LTD	02V0		
			BRITE PLUS ELECTRONICS (SUZHOU) CO LTD	DKV0-3A		
			Various	Various		
3	10	Insulating tape wrapping around the PCB edge (Optional)	3M COMPANY ELECTRICAL MARKETS DIV (EMD)	1350F-1 1350T-1	Min.130°C	cURus
			BONDTEC PACIFIC CO LTD	370S		
			JINGJIANG YAHUA PRESSURE SENSITIVE GLUE CO LTD	PZ CT		
			JINGJIANG JINGYI ADHESIVE PRODUCT CO LTD	JY25-A		
			CHANG SHU LIANG YI TAPE INDUSTRY CO LTD	LY-XX		
13	11	Plug portion	GlobTek	Q-NA(2)	NEMA 5-15, referring to illustration No(s). 7-12 for details.	NR

NOTES:

- 1) Not all item numbers are indicated (called out) in the photos, as their location is obvious.
- 2) "Various" means any type, from any manufacturer that complies with the "Technical data and securement means" and meets the "Mark(s) of conformity" can be used.
- 3) Indicates specific marks to be verified, which assures the agreed level of surveillance for the component. "NR" - indicates Unlisted and only visual examination is necessary. "See 5.0" indicates Unlisted components or assemblies to be evaluated periodically refer to section 5.0 for details.

5.0 Critical Unlisted CEC Components

No Unlisted CEC components are used in this report.

6.0 Critical Features

Recognized Component - A component part, which has been previously evaluated by an accredited certification body with restrictions and must be evaluated as part of the basic product considering the restrictions as specified by the Conditions of Acceptability.

Listed Component - A component part, which has been previously Listed or Certified by an accredited Certification Organization with no restrictions and is used in the intended application within its ratings.

Unlisted Component - A part that has not been previously evaluated to the appropriate designated component standard. It may also be a Listed or Recognized component that is being used outside of its evaluated Listing or component recognition.

Critical Features/Components - An essential part, material, subassembly, system, software, or accessory of a product that has a direct bearing on the product's conformance to applicable requirements of the product standard.

Construction Details - For specific construction details, reference should be made to the photographs and descriptions. All dimensions are approximate unless specified as exact or within a tolerance. In addition to the specific construction details described in this Report, the following general requirements also apply.


1. Spacing - Refer to illustration No(s) 2-3 for details.
2. Mechanical Assembly - Components such as switches, fuseholders, connectors, wiring terminals and display lamps are mounted and prevented from shifting or rotating by the use of lockwashers, starwashers, or other mounting format that prevents turning of the component.
3. Corrosion Protection - All ferrous metal parts are protected against corrosion by painting, plating or the equivalent.
4. Accessibility of Live Parts - For adapter models, all uninsulated live parts in primary circuitry are housed within a non-metallic enclosure constructed with no openings and metal enclosure earthed with ventilation holes other than those specifically described in Sections 4 and 5.
5. Grounding - Class II appliance.
6. Polarized Connection - This product is provided with a polarized power supply connection.
7. Internal Wiring - Final determination in end-product evaluation.
8. Schematics - Refer to Illustration No(s). 4-5 for schematics & PCB layout requiring verification during Field Representative Inspection Audits.
9. Markings - The product is marked as follows: brand name, model number, electrical ratings, manufacturer. Refer to Illustration No. 6 for details.
10. Cautionary Markings - Refer to illustrations No. 6 for details.
11. Safety Instructions - Accompanying Documents are provided for some critical issue like technical data, safety warnings, necessary information to set up, but further evaluation is needed on end product level.

7.0 Illustrations

Illustration 1 - Model list

Model	Rated output voltage range	Max. rated output current	Max. rated output power	Transformer designation
GT*41061-*12*	5-12Vdc	3.6A	18W	TF001
GT*41061-*18*	12.1-18Vdc	1.49A	18W	TF002
GT*41061-*24*	18.1-24Vdc	1.0A	18W	TF003
GT*41061-*30*	24.1-30Vdc	0.75A	18W	TF004

Illustration 2 - INSULATION DIAGRAM

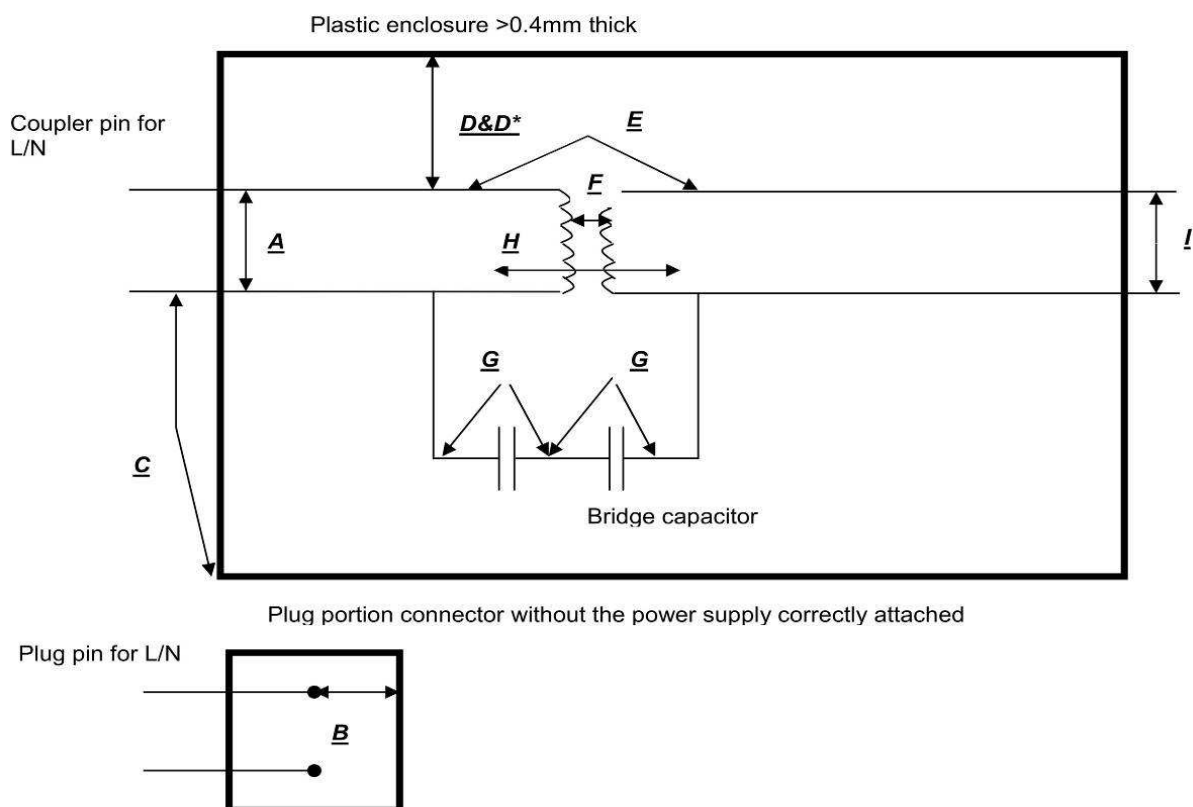

7.0 Illustrations


Illustration 3 - TABLE: Insulation diagram (measured values)

Pollution degree..... :		2		—					
Overvoltage category..... :		II		—					
Altitude..... :		3000m		—					
Additional details on parts considered as applied parts..... :		<input checked="" type="checkbox"/> None <input type="checkbox"/> Areas _____ (See Clause 4.6 for details)		—					
Area	Number and type of Means of Protection: MOOP, MOPP	CTI (IIIb, unless is known)	Working voltage		Required creepage (mm)	Required clearance (mm)	Measured creepage (mm)	Measured clearance (mm)	Remarks
			Vrms	Vpk					
A	BOP	IIIb	240	340	3	1.9 ¹	3.1	3.1	Opposite polarity of mains part
B	2MOOP	IIIb	240	340	4.8	4.6 ¹	5.6	5.6	Plug pin-out on the connector side to accessible part when the plug portion is plugged in the socket without the power supply correctly attached.
C	2MOOP	IIIb	240	340	4.8	4.6 ¹	9.0	9.0	Mains part (plug portion) to outer enclosure (accessible position during normal use)
D	2MOPP	IIIb	240	--	7.9 ²	5.0	8.0	8.0	Internal mains part to accessible outer enclosure with insulating tape around the PCB edge
D*	2MOOP	IIIb	240	340	4.8	4.6 ⁵	5.1	5.1	Internal mains part to accessible outer enclosure without insulating tape around the PCB edge
E	2MOPP	IIIb	240 ³	--	7.9 ²	5.0	8.0 ⁴	8.0 ⁴	Mains part to secondary circuits (Optocoupler)
F	2MOPP	IIIb	276 ¹	--	8.7 ²	7.0	10.0 ⁵	10.0 ⁵	Mains part to secondary circuits (Transformer)
G	MOPP (Each) x 2	IIIb	240 ¹	--	4.0 ²	2.5	4.1	4.1	Mains part to secondary circuits (Y capacitor x 2)
H	2MOPP	IIIb	240 ¹	--	7.9 ²	5.0	8.7 ⁶	8.7 ⁶	Mains part to secondary circuits (On PCB trace)
I	2MOOP	IIIb	--	Max. 30Vdc	--	--	--	--	Accessible part per 8.4.2 c)
Note: 1) Multiplication factor for MOOP: 1.14; Multiplication factor for MOPP: 1.00. 2) Linear interpolation is applied to the determination of required creepage. 3) The working voltage is highest measured value which acquired by testing all the models listed in the report at the rated input voltage, but not less than the rated input voltage. 4) The minimum creepage and clearance is selected from all the types of optocouplers. 5) The transformer core regarded as primary conductor is wrapped with 2 layers of insulating tape and the secondary adopts the jump lead wire soldering. 6) There is a slot min. 1 mm wide between primary pins and secondary pins of optocoupler.									

7.0 Illustrations

Illustration 6 - Marking label

The marking plates of the other models listed in this report are identical with below except model name and output parameter.

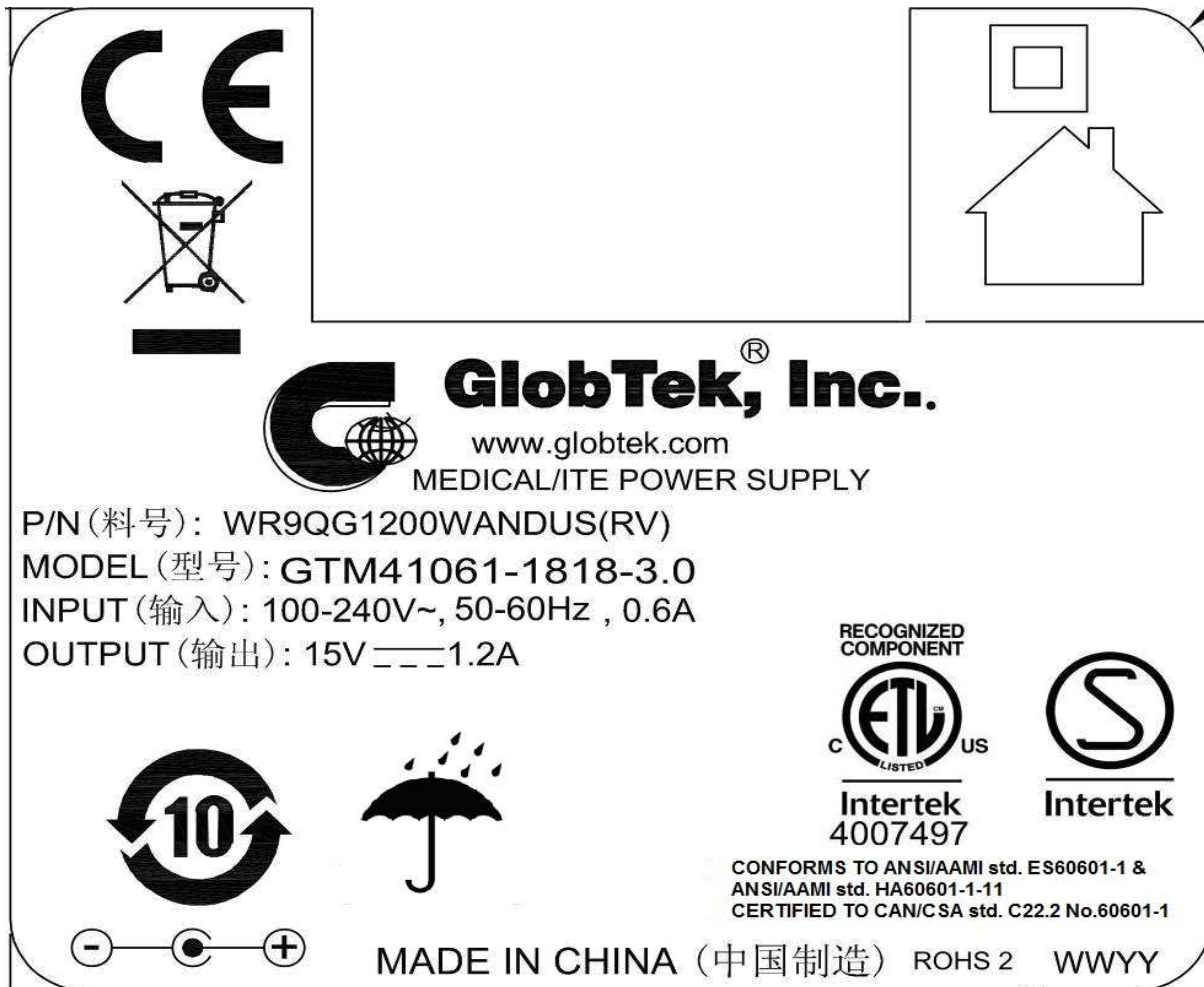

7.0 Illustrations

Illustration 7 - Appendix: Equipment's combined with NEMA 1-15 plug portion

KEY:

- | | | | |
|----|--------------------------------|-----|--------------------|
| √ | = Complies. | G | = General comment |
| E | = Further evaluation required | N/A | = Not applicable |
| E√ | = Once "E" is found acceptable | T | = Testing required |
| F | = Non-compliance | TF | = Test failed |

Section	Key	Comment
FORWARD		
Introduction		
1		Scope
1.1-1.4	G	The device under evaluation is an integral plug for medical power supply GT*41061-*** whose input rated 100-240V~, 50-60Hz, 0.6A. The plug is evaluated according to rated input.
2		Glossary
2.1-2.38	G	Noted.
3		Components
3.1-3.4	G	Noted
4		Units of Measurement
4.1	G	Noted
5		Reference
5.1	G	Noted
CONSTRUCTION		
ALL DEVICES		
6		General
6.1	√	According to declared reasonable condition, 100-240VAC, 50-60Hz, has been considered in all following test.
6.2	√	Plug for AC use only
7		Configurations
7.1	√	1-15P plug applied.
8		Insulating Materials
8.1		General
8.1.1	√	All parts that act as the electrical insulation or enclosure are made of plastic material. See 8.2.1
8.1.2	N/A	Vulcanized fiber is not provided
8.2		Flammability
8.2.1	√	The insulating material required HB or more. For detailed parts, see report of end product)
8.3		Electrical properties
8.3.1	√	Exception No. 1: No information according to above table info. The insulating material has a CTI 3 (Required 3), so it need NOT comply with Comparative Tracking Index Test, Section 55.
8.3.2	√	Exception No. 2: The insulating material has a HWI 3, (required HWI value is 4 when material class is V-0). According to 8.1.2 (UL746D) and reasonable usage, reasonable arcing occurs in normal use. We are of the opinion that it need NOT comply with Glow Wire Test, see Section 56. Exception No. 3: The insulating material has a HAI 2. (required HWI value is 4 when material class is V-0. or check if the thickness), since no arcing in normal use, so it need not comply with High-Current Arc Resistance to Ignition Test, Section 57.
8.4		Thermal properties
8.4.1	√	All the RTI rating of the insulating materials are higher than 80 degree (C)
8.5		Vulcanized fiber

7.0 Illustrations

Illustration 8 - Appendix: Equipment's combined with NEMA 1-15 plug portion (cont.)

Section	Key	Comment
8.5.1	N/A	No Vulcanized fiber is provided
8.5.2	N/A	No Vulcanized fiber is provided
8.6		Sealing compounds
8.6.1-8.6.2	N/A	Sealing compound is not provided, no need to comply with relevant requirement involved in ASTM 28.
8.7		Fuse enclosures
8.7.1-8.7.2	N/A	Fuse is not provided
9		Enclosure
9.1		General
9.1.1	√	Live parts of plug parts are protected against exposure to contact by persons when fully assembled using all essential parts. Exception no. 2: for fixed wiring.
9.1.2-9.1.3	N/A	No accessible dead-metal parts
9.1.4	√	The probe shown in Figure 9.1 is used to judge the accessibility of a live or dead-metal part. The applied force is not more than 13.3N.
9.1.5-9.1.7	N/A	No such separable part
9.2		Male faces and wire terminations
9.2.1	N/A	Not a 15 or 20A attachment plug or current tap
9.2.2	N/A	There is no exposed live part.
9.2.3	N/A	No such parts
9.2.4-9.2.5	√	Probe not access to live parts. The cover is securely fixed for all acceptable wiring.
9.2.6	√	The face plate is secure with the back part.
10		Current-carrying Parts
10.1		General
10.1.1	√	Iron or steel is not used for current-carrying parts.
10.1.2	√	The current-carrying parts are not able to be turned by means of general tools due to the appliance shroud mounted on Evaluated appliance.
10.1.3	N/A	No such uninsulated live parts except for female contact of connector
10.2		Contacts (applying to the connector)
10.2.1	N/A	Female contacts of the connector cannot be touched by the probe. Others parts are covered by exception no. 3
11		Grounding and Dead Metal Parts
11.1-11.10	N/A	No grounding parts
12		Terminals
12.1-12.4		No terminals for end user
13		Cord Entry and Strain Relief
13.1-13.5	N/A	Flexible cord part are considered in the end appliances.
14		Spacings
14.1	√	The spacing through air between uninsulated live parts of opposite polarity and between uninsulated live parts and exposed external surface is measured more than 2mm (required 3/36 inch, 1,2mm) for a device rated 250V or less.
14.2	N/A	No such isolated dead-metal part
15		Assembly
15.1		General
15.1.1	√	Pre-wired in factory

7.0 Illustrations

Illustration 9 - Appendix: Equipment's combined with NEMA 1-15 plug portion (cont.)

Section	Key	Comment
15.1.2	√	Electrical contact is reliably maintained at any point
15.1.3	√	Live parts is protected against exposure to persons
15.1.4	N/A	Not multiple outlet device
15.1.5	N/A	Female contacts of the connector can be mated with the inlet in right way without exposure of the blades
15.2		Grounding and polarization
15.2.1-15.2.4	N/A	No grounding
15.3		Mating and interchangeability
15.3.1	√	The electrical continuity is automatically established.
15.3.2-15.3.6	√	1-15P receptacles ensuring.
15.4		Fuseholders
15.4.1-15.4.8	N/A	Fuseholder is not provided
15.5		Switches
15.5.1	N/A	The switch is provided between coupler 1 and coupler 2. but it is a information
ATTACHMENT PLUGS AND INLETS (for plug only)		
16		Insulating material
16.1	√	The enclosure is measured min. 2.1 mm.
17		Enclosure
17.1		General
17.1.1	N/A	Not a general use plug.
17.1.2	√	Measured 44 mm.
17.1.3	N/A	Not a 50A plug
17.2		Grip
17.2.1	N/A	See section 69
17.3		Face size
17.3.1	√	Larger than figure 17.1
18		Current carrying parts
18.1	N/A	Not a folded-over plug.
18.2	√	Dimensional requirements fulfilled.
19		Grounding and dead metal parts
19.1-19.4	N/A	No grounding or dead metal parts.
20		Terminals and leads
20.1-20.5	N/A	All the assembly are pre-wired in factory
21		Assembly
21.1	√	The blades are held securely in place
21.2	N/A	Not a inlet
21.3-21.4	N/A	The device under evaluate is a plug part not inlet or surface mounting.
21.5	N/A	Not for radio antenna or ground.
22		Weatherproof type
22.1-22.2	N/A	Not weatherproof type
23-26	N/A	CONNECTORS
27-37	N/A	RECEPTACLES
		SELF-CONTAINED RECEPTACLES FOR USE WITHOUT A SEPARATE OUTLET BOX

7.0 Illustrations

Illustration 10 - Appendix: Equipment's combined with NEMA 1-15P plug portion (cont.)

Section	Key	Comment
38-44	N/A	These sections are applicable for self-contained receptacles.
		CURRENT TAPS
45	N/A	The section is applicable for current taps only
		FLATIRON AND APPLIANCE PLUGS
46-53	N/A	These sections are applicable for flatiron and appliance plugs.
PERFORMANCE		
		GENERAL
54		Representative Devices
54.1-54.7	G	Noted.
		ALL DEVICES
55		Comparative Tracking Index Test
55.1	N/A	Refer to Exception No. 2 of 8.3.2. Not main tests but the test is considered
56		Glow Wire Test
56.1-56.2	N/A	Refer to Exception No. 2 of 8.3.2, Not main tests but the test is considered
57		High-Current Arc Resistance to Ignition Test
57.1-57.6	G	Refer to Exception No. 3 of 8.3.2
58		Mold Stress Relief
58.1-58.2	T	All devices are placed in air oven maintained at a 80oC for 7 hours. After 58.2, there is not any warpage, shrinkage or other distortion.
58.3	T	Refer to data sheet. Repeat dielectric voltage-withstand test as described in section 60. Not required to be subjected to the humidity conditioning described in 60.1.2.
59		Moisture Absorption Resistance
59.1-59.2	T	Refer to data sheet
60		Dielectric Withstand Test
60.1-60.2	T	Refer to data sheet
61		Accelerated Aging Tests
61.1		General
61.1.1	G	Exception to 8.4.1 for other material is not applicable for the devices under evaluation
61.2		Rubber, EPDM, and TEE compounds
61.2.1-61.2.4	N/A	Not a rubber , EPDM, and TEE compounds
61.3		PVC compounds and copolymers
61.3.1-61.3.2	G	See 61.1.1 shown as above
62		Insulation Resistance Test
62.1-62.6	T	Refer to data sheet
63		Conductor Secureness Test
63.1-63.2	N/A	No wire leads provided.
64		Tightening Torque Test
64.1-64.2	N/A	Not provide any wire-binding screw
	N/A	ATTACHMENT PLUGS
65		General
65.1	G	Noted.
66		Security of blades test

7.0 Illustrations

Illustration 11 - Appendix: Equipment's combined with NEMA 1-15P plug portion (cont.)


Section	Key	Comment
66.1-66.2	T	Refer to data sheet
67		Secureness of cover test
67.1-67.2	T	Refer to data sheet
68		Crushing test
68.1-68.2	T	Refer to data sheet
69		Attachment plug grip test
69.1-69.9	T	Refer to data sheet
70		Integrity of assembly test
70.1-70.2	N/A	Cord part shall be considered in the end appliance.
71		Self-hinge Flexing test
71.1-71.3	N/A	Not self-hinge type
72		Terminal temperature test
72.1-72.4	N/A	No terminal for end user.
73		Fuse-holder temperature test
73.1-73.8	N/A	No fuse-holder applied.
74-79	N/A	Pin type terminal
80-85	N/A	INLET (applying for inlet)
86-103	N/A	CONNECTORS
104-150	N/A	RECEPTACLES
		CURRENT-TAPS
		All devices
151-152	N/A	These sections are for current-taps
		Flatiron and appliance plugs.
153-161	N/A	These sections are applicable for flatiron and appliance plugs.
RATINGS		
162		Details
162.1	G	According to exception no. 2, rating is not required. The special-use device is not intended to ship out solely. (Note: plug is mounted in evaluated appliance).
162.2	√	Rating of 1A 120V~ is evaluated
162.3	√	0.5HP rated.
162.4-162.7	N/A	Not have the specified devices
MARKINGS AND INSTRUCTIONS		
163		General
163.1-163.2	G	The location of the catalog number is not prohibited from appearing according to exceptions of table 163.1 and 163.2
164		Identification and marking of terminals
164	G	No any grounding parts and terminals
SUPPLEMENT SA		(reserved for future use)
SUPPLEMENT SB		ENCLOSURE TYPES FOR ENVIRONMENTAL PROTECTION
SB1-SB7	N/A	The requirements of SB don't apply to the device under evaluation for it's intended for indoor use only (refer to SB1.1)
SUPPLEMENT SC		MARINE SHORE POWER INLETS

7.0 Illustrations

Illustration 12 - Appendix: Equipment's combined with NEMA 1-15P plug portion (cont.)

Section	Key	Comment
SC1-SC12	N/A	These sections are for marine shore power inlets
SUPPLEMENT SD		HOSPITAL GRADE DEVICES
SD1-SD30	N/A	These sections are for hospital grade devices

Appendix: Dimensions of NEMA 1-15P plug portion

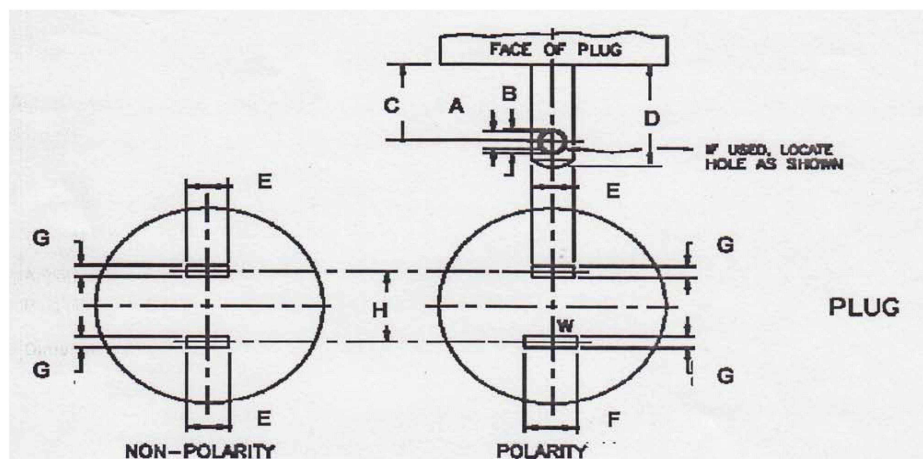

Symbol	Requirement (inch)	Measured (inch)	Symbol	Requirement (inch)	Measured (inch)
A	0.120 – 0.130	0.123	E	0.240 – 0.260	0.248
B	0.151 – 0.161	0.157	F	0.307 – 0.322	--
C	0.449 – 0.479	0.466	G	0.055 – 0.065	0.057
D	0.625 – 0.718	0.656	H	0.495 – 0.505	0.498
Perimeter faces to the plug blades shall not be less than 7.9 mm (intended for use with children's toys) or 5.1 mm from any point of either blade					12.39

8.0 Test Summary			
Evaluation Period	2013-06-03 ~ 2013-06-24		Project No. 130501374SHA
Sample Rec. Date	3-Jun-2013	Condition	Prototype
Sample ID	0130603-77-001		
Test Location	Building No.86, 1198 Qinzhou Road (North), Shanghai 200233, China		
Test Procedure	Testing Lab		
Determination of the result includes consideration of measurement uncertainty from the test equipment and methods. The product was tested as indicated below with results in conformance to the relevant test criteria.			
The following tests were performed:			
Test Description	Medical Electrical Equipment, Part 1: General Requirements for Basic Safety and Essential Performance (ANSI/AAMI ES60601-1 Issued: 2006/03/09: 2005 Version (R2012); with AMD C1: 2009, AMD C2: 2010 & CAN/CSA-C22.2 No.60601-1 Issued: 2008/02/01; with COR 2: 2011/06/01)		
	Clause		
Power Input	4.11		
Humidity Preconditioning	5.7		
Accessible Parts	5.9.2		
Legibility of Markings	7.1.2		
Durability of Markings	7.1.3		
Plug Voltage and/or Energy	8.4.3		
Working Voltage Measurement	8.5.4		
Leakage Current Test terminations	8.7.4		
Dielectric Strength Means	8.8.3		
Ball Pressure Test	8.8.4.1		
Creepage & Clearance Measurements	8.9.4		
Excessive Temperature	11.1		
Single Fault Conditions	13.2		
Push Test	15.3.2		
Drop Test	15.3.4		
Moulding Stress Relief	15.3.6		
Transformer Short-Circuit	15.5.1.2		
Transformer Overload	15.5.1.3		
Transformer Dielectric Strength	15.5.2		

Test Description	Medical electrical equipment, Part 1-11: General requirements for basic safety and essential performance - Collateral Standard: Requirements for medical electrical equipment and medical electrical systems used in the home healthcare environment (ANSI/AAMI HA60601-1-11 Issue:2011/12/12 Ed:1)
	Clause
Environmental conditions of transport and storage between uses	4.2.1
Environmental operating conditions	4.2.2
Mechanical strength for non-TRANSIT-OPERABLE ME EQUIPMENT	10.1.2

8.1 Signatures			
A representative sample of the product covered by this report has been evaluated and found to comply with the			
Completed by:	Jamie Wu	Reviewed by:	Karl Zhong
Title:	Project engineer	Title:	Reviewer
Signature:	<i>Signature on file</i>	Signature:	<i>Signature on file</i>

9.0 Correlation Page For Multiple Listings

The following products, which are identical to those identified in this report except for model number and Listee name, are authorized to bear the ETL label under provisions of the Intertek Multiple Listing Program.

BASIC LISTEE	GlobTek, Inc.
Address	186 Veterans Dr. Northvale, NJ 07647 USA
Country	USA
Product	Medical Power Supply

MULTIPLE LISTEE 1	None
Address	
Country	
Brand Name	

ASSOCIATED MANUFACTURER	
Address	
Country	

MULTIPLE LISTEE 1 MODELS	BASIC LISTEE MODELS

MULTIPLE LISTEE 2	None
Address	
Country	
Brand Name	

ASSOCIATED MANUFACTURER	
Address	
Country	

MULTIPLE LISTEE 2 MODELS	BASIC LISTEE MODELS

MULTIPLE LISTEE 3	None
Address	
Country	
Brand Name	

ASSOCIATED MANUFACTURER	
Address	
Country	

MULTIPLE LISTEE 3 MODELS	BASIC LISTEE MODELS

10.0 General Information

The Applicant and Manufacturer have agreed to produce, test and label ETL Listed products in accordance with the requirements of this Report. The Manufacturer has also agreed to notify Intertek and to request authorization prior to using alternate parts, components or materials.

COMPONENTS

Components used shall be those itemized in this Intertek report covering the product, including any amendments

LISTING MARK

The ETL Listing mark applied to the products shall either be separable in form, such as labels purchased from Intertek, or on a product nameplate or other media only as specifically authorized by Intertek. Use of the mark is subject to the control of Intertek.

The mark must include the following four items:

- 1) applicable country identifiers "US" and/or "C" or "US", "C" and "EU"
- 2) the word "Listed" or "Classified" or "Recognized Component" (whichever is appropriate)
- 3) a control number issued by Intertek
- 4) a product descriptor that identifies the standards used for certification. Example:

For US standards, the words, "Conforms to" shall appear with the standard number along with the word, "Standard" or "Std." Example: "Conforms to ANSI/UL Std. XX."

For Canadian standards, the words "Certified to CAN/CSA Standard CXX No. XX." shall be used, or abbreviated, "Cert. to CAN/CSA Std. CXX No. XX."

Can be used together when both standards are used.

Note: A facsimile must be submitted to Intertek, Attn: Follow-up Services for approval prior to use.

The facsimile need not have a control number. A control number will be issued **after signed Certification Agreements** have been received by the Follow-up Services office, approval of the facsimile of your proposed Listing Mark, satisfactory completion of the Listing Report, and scheduling of a factory assessment in your facility.

MANUFACTURING AND PRODUCTION TESTS

Manufacturing and Production Tests shall be performed as required in this Report.

FOLLOW-UP SERVICE

Periodic unannounced audits of the manufacturing facility (and any locations authorized to apply the mark) shall be scheduled by Intertek. An audit report shall be issued after each visit. Special attention will be given to the following:

1. Conformance of the manufactured product to the descriptions in this Report.
2. Conformance of the use of the ETL mark with the requirements of this Report and the Certification Agreement.
3. Manufacturing changes.
4. Performance of specified Manufacturing and Production Tests.

In the event that the Intertek representative identifies non-conformance(s) to any provision of this Report, the Applicant shall take one or more of the following actions:

1. Correct the non-conformance.
2. Remove the ETL Mark from non-conforming product.
3. Contact the issuing product safety evaluation center for instructions.

10.1 Evaluation of Unlisted Components

Because Unlisted Components are uncontrolled, and they do not fall under a third party follow up program, Intertek may require these components to be tested and/or evaluated at least once annually, more often for certain components, as part of the independent certification process. The Unlisted Components in Section 5.0 require testing and/or evaluation as indicated.

Note to Intertek Follow Up Inspector: The Component Evaluation Center, CEC, will notify you in writing when these components must be selected and sent to the CEC for re-evaluation

Ship the samples to:
Intertek Testing Services Shanghai Limited
ETL Component Evaluation Center
Building No. 86, 1198 Qinzhou Road (North)
Shanghai 200233, China
Attn: Ms. Dansy Xu

Sample Disposition: Due to the destructive nature of the testing, all samples will be discarded at the conclusion of testing unless, the manufacturer specifically requests the return of the samples. The request for return must accompany the initial component shipment.

11.0 Manufacturing and Production Tests

The manufacturer agrees to conduct the following Manufacturing and Production Tests as specified:

Required Tests

Dielectric Voltage Withstand Test

11.1 Dielectric Voltage Withstand Test

Method

One hundred percent of production of the products covered by this Report shall be subjected to a routine The test shall be conducted on products, which are fully assembled. Prior to applying the test potential, all The test voltage specified below shall be applied between primary circuits and accessible dead-metal parts. The

Test Equipment

The test equipment shall incorporate a transformer with an essentially sinusoidal output, a means to indicate the The test equipment shall incorporate a voltmeter in the output circuit to indicate directly the applied test potential If the rated output of the test equipment is 500VA or more, the applied test potential may be indicated by either:

Products Requiring Dielectric Voltage Withstand Test:

<u>Product</u>	<u>Test Voltage</u>	<u>Test Time</u>
Between mains part and secondary circuits	4000V	1 s

